Prime Core Dynamics
support@primecoredynamics.com

Louisiana, USA

COC# 145927
Lab # 214653
Date Rec'd 9/25/2026
Report Issued 10/12/2026

Certificate of Analysis



Project
Compound hCG
Label Claim 10000 IU
Batch/Lot HCG-10000IU-A01

Analyte	Result	Units	LOQ	% of Label	Method	Date	CAS
Peptides & Bioactives							
Chromatographic purity	>99.9	%	1		HPLC-UV/MS	10/5/2026	
hCG	11,200	IU	.1	111.9	HPLC-UV-MS	10/5/2026	9002-61-3
Mass Spectral Match	ID Confirmed				HPLC-UV-MS	10/5/2026	

The data presented are from the analysis of the sample shown and meet Krause Analytical internal quality assurance criteria unless otherwise flagged.
Data is not for regulatory compliance nor diagnostic use.
Methods shown reference current Krause Analytical SOPs
ND - Not detected LOQ - limit of quantification
OCH - above calibrated range OCL - below calibrated range
All values reported on a per vial basis unless otherwise noted
Copyright © 2026 Krause Analytical LLC. All rights reserved.

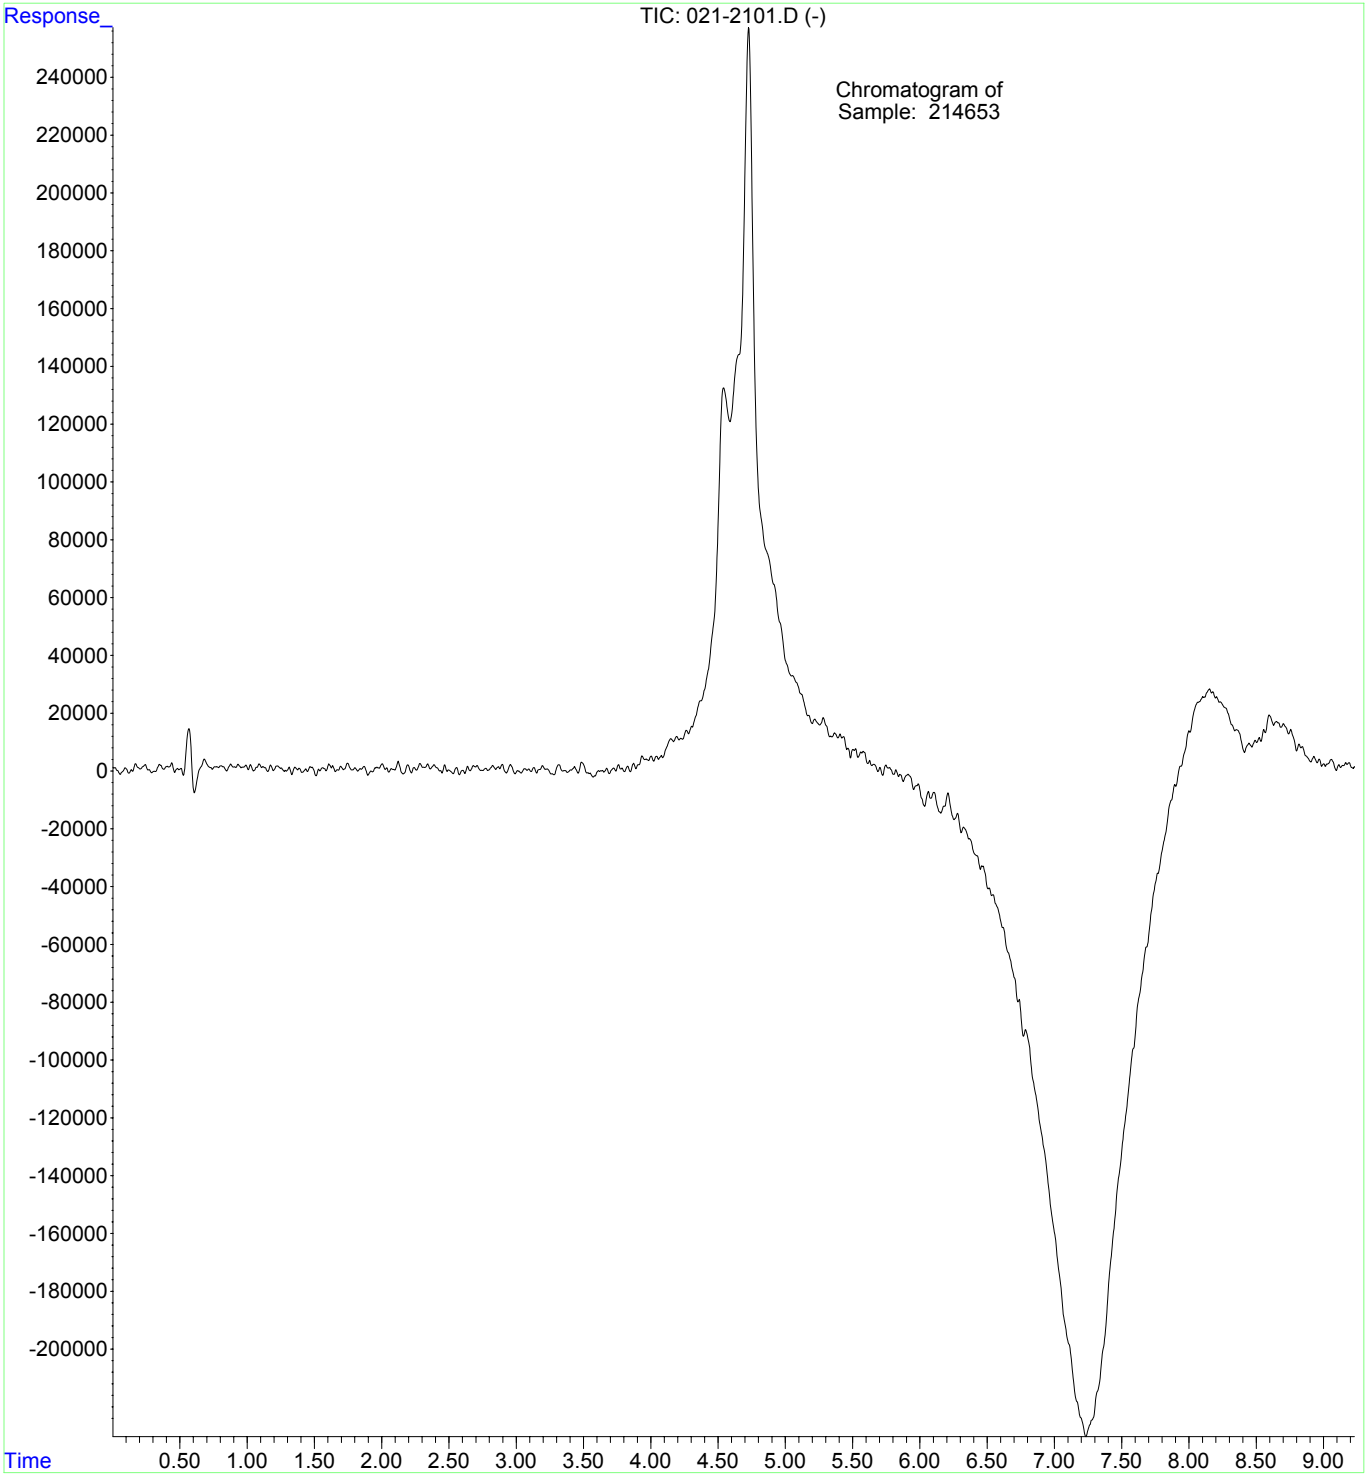
Respectfully submitted,

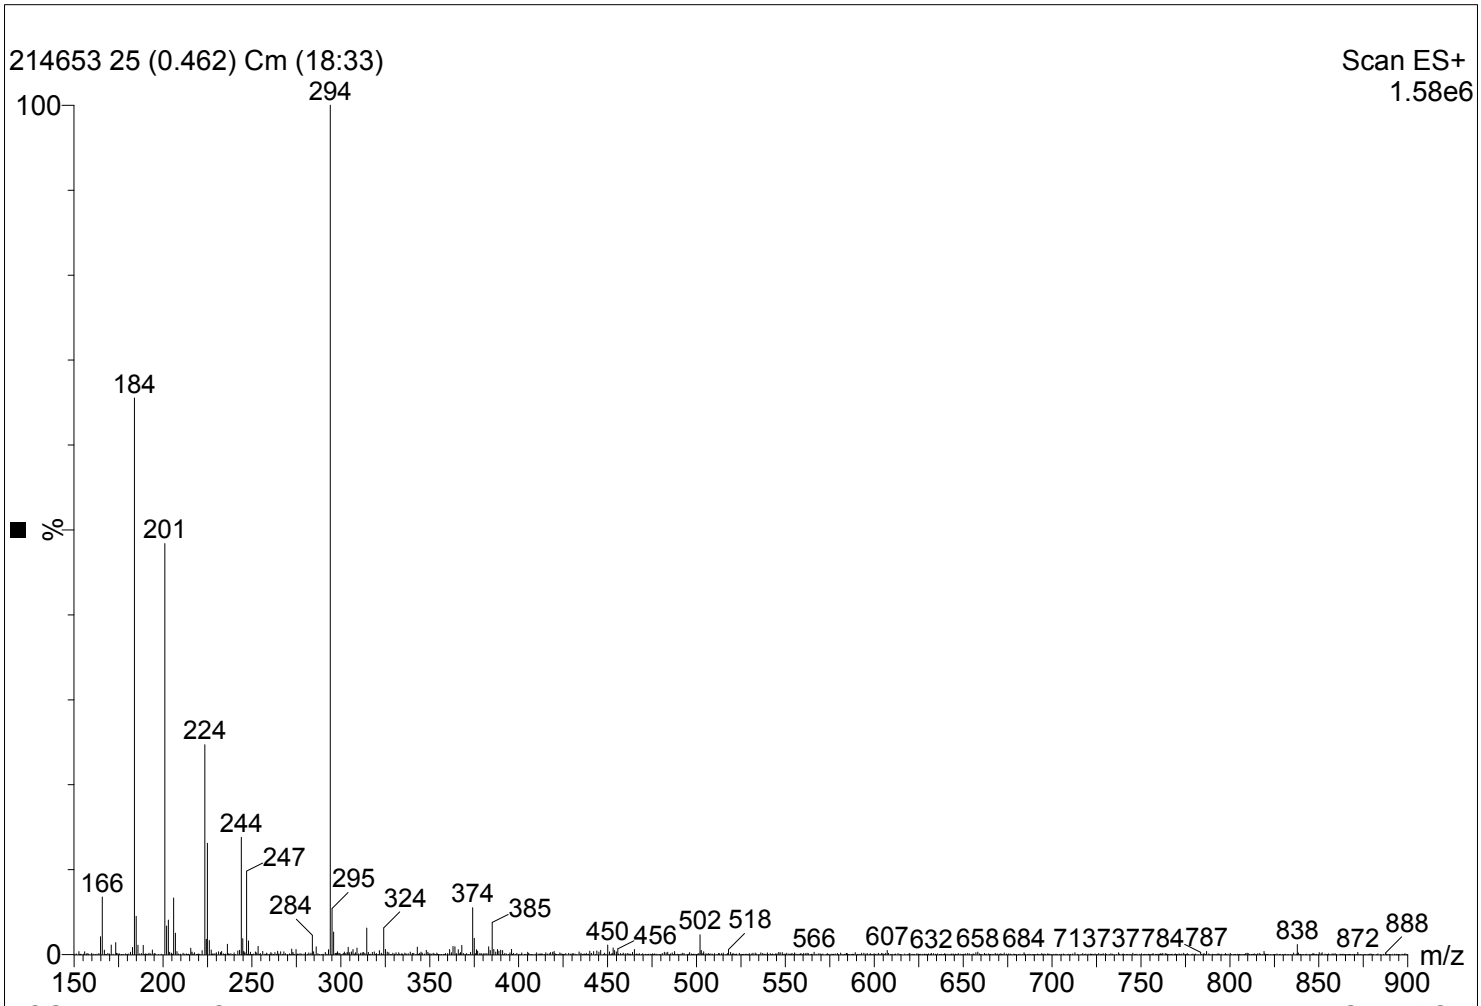
Mark C. Krause
Laboratory Director

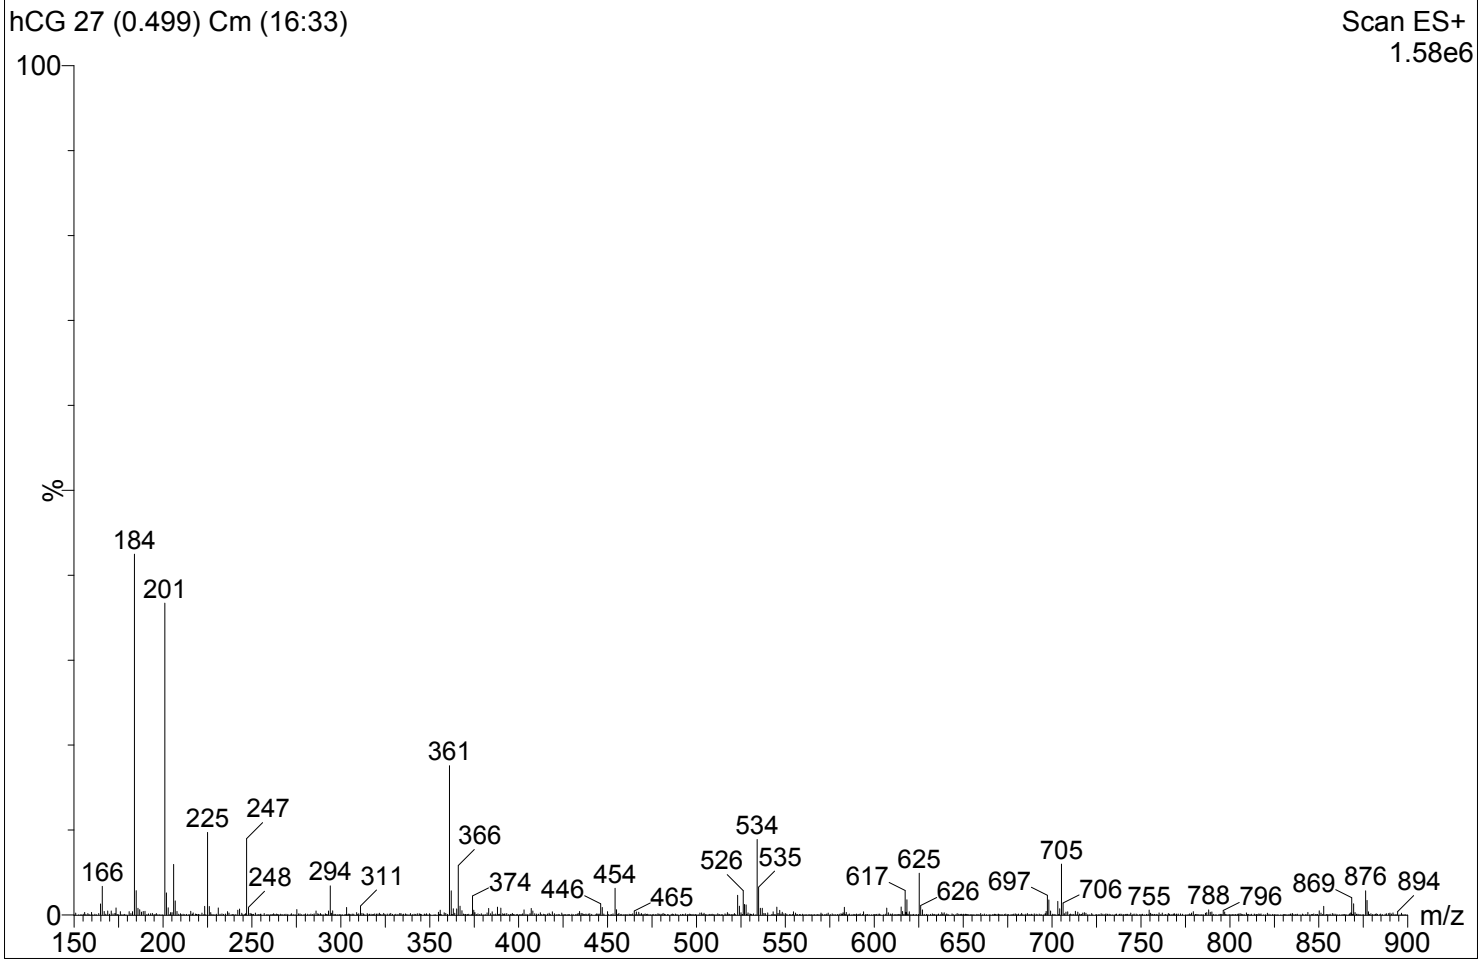
****

CHROMATOGRAM

****




214653 25 (0.462) Cm (18:33)
Scan ES+
1.58e6
100
%
0
294
184
201
224
244
247
166
295
284
324
374
385
450
456
502
518
566
607
632
658
684
713
737
784
787
838
872
888
m/z
150
200
250
300
350
400
450
500
550
600
650
700
750
800
850
900


hCG 27 (0.499) Cm (16:33)
Scan ES+
1.58e6
100
%
0
184
201
361
225
247
366
166
248
294
311
374
446
454
465
526
534
535
617
625
626
697
705
706
755
788
796
869
876
894
m/z
150
200
250
300
350
400
450
500
550
600
650
700
750
800
850
900